Yocom-McColl Testing Laboratories, Inc.
540 West Elk Place • Denver, Colorado 80216-1823 USA
PHONE (303) 294-0582 • FAX (303) 295-6944
EMAIL: ymccoll@ymccoll.com

Optical Fiber Diameter Analyser (OFDA 100)
Micron Test Report

Herzog-Alpakas/Christina & Andreas Klövekorn
Herzog-Erich-Weg 22
49685 Drantum, Niedersachsen Germany

Date: 02/26/19
Test No: 972815

Animal and Sample Description

Animal Name:	BUT Luna Mae	**Animal ID:**	276094800011035
Breed:	Alpaca(Huacaya)	**Sample Location:**	Blanket
Sex:	Female	**Sample Date:**	02/18/19
Color:	White	**Age:**	06/20/18

Laboratory Data

Mean Fiber Diameter:	18.5 microns	**Fibers Greater Than 30 microns:**	0.6 %
Standard Deviation:	3.7 microns	**Comfort Factor:**	99.4 %
Coefficient of Variation:	19.9 %	**Mean Curvature:**	41.0 deg/mm
Spin Fineness:	17.8 microns	**SD Curvature:**	30.3 deg/mm

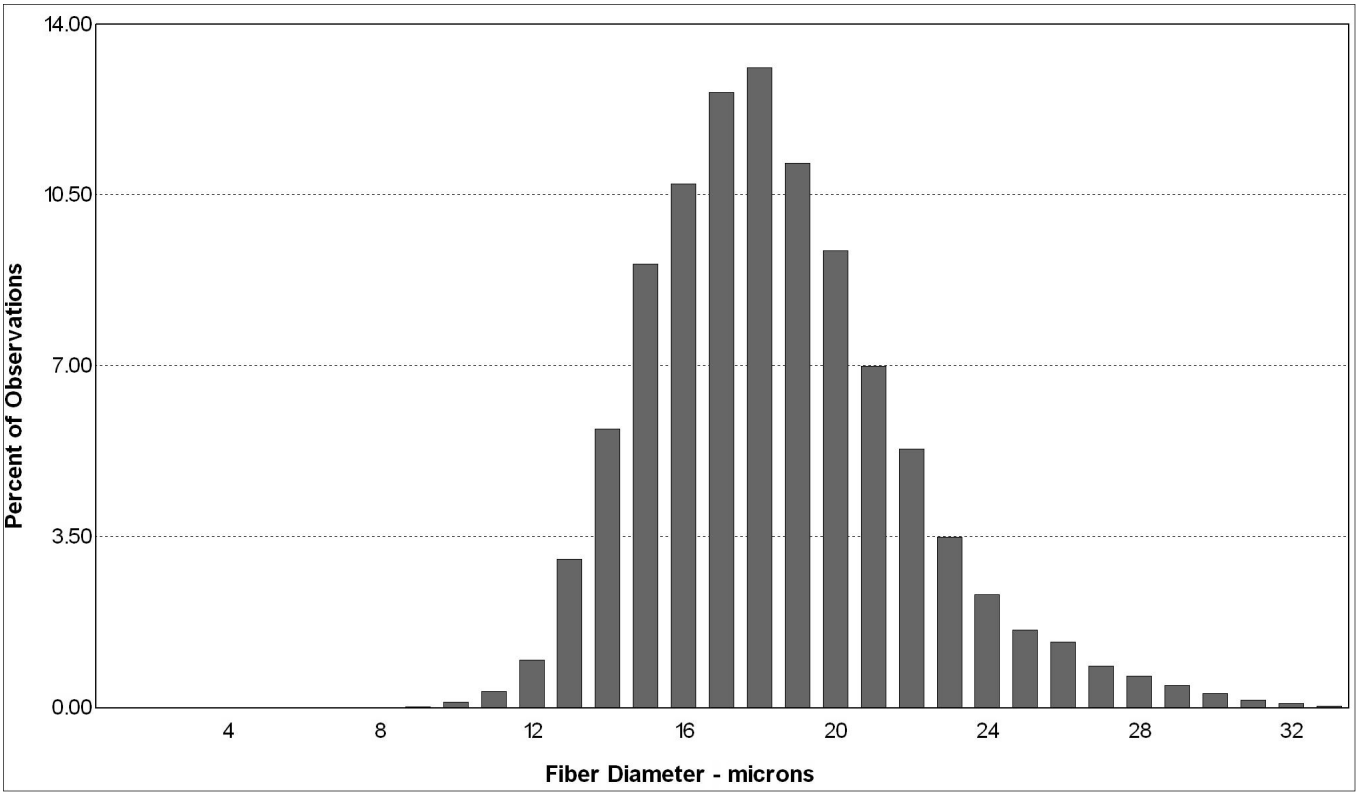

This Test Performed According to I.W.T.O Method 47